DIRECTION FOR USE

DILUTION 2%

Alkasept Ultra

Universal cleaner

Description

For the cleaning by immersion of all medical instuments. Before use, check the expiration date on the bottle. Store container tightly closed, in its original packaging and labeling. Do not mix with other products.

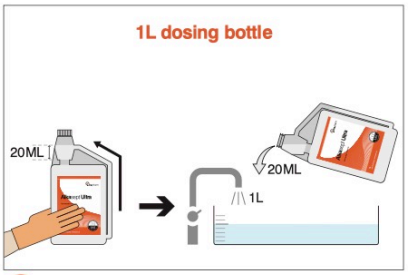

1 Press the sides of the bottle to automatically obtain a dose of 20mL. Pour 20mL for 1L of tap water. (≃20°C)

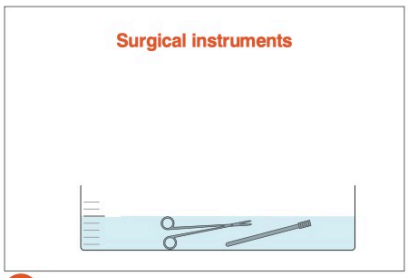

2 Totally immerse opened and dismantled instruments. Brush until visual cleanliness.
For Ultrasonic baths: a minimum of 5 minutes in the bath.

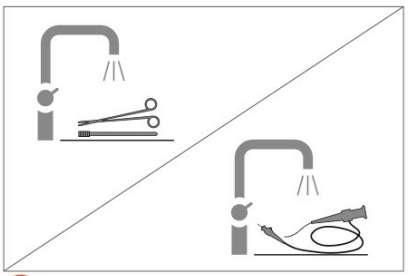

3 Rinse thoroughly with tap water.

Instrument Care

1. Avoid contact corrosion by seperating stainless steel from NON stainless steel instruments and disinfect seperatley.

2. Discard corroded instruments.(rust particles are transferred from one instrument to another during cleaning, diinfecting and sterilising).

3. To help preserve instrument life a second and final rinse using Demineralised Water is recommended.

Always follow the manufacturers instructions.

4 **Renew the preparation when soiled and at least once a day.**

Then proceed to the steps of disinfection and/or sterilisation of medical devices before reuse.

Packaging

1L dosing bottle

Cautionary notes

Wear eye & hand protection.

Before use, read the label and product information.

WARNING

Storage conditions

Store container tightly closed, in its original packaging and labeling.



Alkapharm
Targeting Infection

Manufactured in the UK by:
Qualkem Ltd.
Macon Way,
Crewe,
Cheshire. CW1 6YU
United Kingdom
Tel: +44 (0) 1270 587616
www.qualkem.com

Access health and safety data sheets online

PROFESSIONAL USE

MEDICAL DEVICES

CE MD

This product is a Medical Device.